

Une toute nouvelle étude concerne les appareils mobiles de chez IQair sur l'élimination des virus. Un test indépendant prouve le taux d'élimination du virus de 99,9% avec les IQAir HealthPro. Un laboratoire de test européen indépendant accrédité (Airmid Healthgroup of Ireland) a récemment évalué la capacité des modèles IQAir HealthPro à éliminer les virus en suspension dans une pièce. Les tests ont montré que les modèles HealthPro 100 et 250 ont atteint **une réduction de 99,9%** des virus en suspension dans l'air dans une pièce de 28,5 m<sup>3</sup> en moins de 10 minutes. Le test a été réalisé avec des virus H1N1, qui sont dans la même gamme de taille que SARS-CoV-2 et utilisé par les laboratoires de test comme substitut pour les virus corona (l'utilisation réelle du SARS-CoV-2 n'est pas autorisée dans de tels tests d'efficacité d'élimination).



<b>Customer Name</b>	IQAir AG
<b>Customer Address</b>	Blumenfeldstrasse 10 CH-9403 Goldach Switzerland
<b>Contact</b>	Mark Mihara
<b>Test Requested</b>	To assess the impact of the air purifier on Influenza A (H1N1) virus in a decay test
<b>Sample Description</b>	IQAir HealthPro 250
<b>Number of Samples</b>	3
<b>Date of Receipt</b>	7 <sup>th</sup> April 2020
<b>ASC Code</b>	ASC003932
<b>Report Number</b>	ASCR092408v2
<b>Report Date</b>	18 <sup>th</sup> June 2020



## Contents

1. Purpose .....	3
2. Test Item Description .....	3
3. Materials and Methods.....	3
4. Protocol .....	4
5. Results and Discussion.....	6
6. Conclusion.....	9
7. Additional Products.....	9
8. References .....	9
9. Amendment History .....	10

## 1. Purpose

---

This report outlines the results following the assessment of the IQAir HealthPro 250 air purifier in removing airborne Influenza A (H1N1) from a 28.5 m<sup>3</sup> environmental test chamber.

## 2. Test Item Description

---

The IQAir HealthPro 250 air purifier was sent by IQAir to **airmid healthgroup** and was received on 07 April 2020 (Figure 2.1).



**Figure 2.1.** IQAir HealthPro 250 air purifier tested at **airmid healthgroup**

## 3. Materials and Methods

---

### 3.1. Materials

- Influenza A (H1N1; A/PR/8/34)
- Influenza A Virus Capture ELISA
- Influenza A Virus Transport Medium

### 3.2. Influenza A

Influenza virus infection is one of the most common, highly contagious infectious diseases and it can occur in people of any age. Influenza A viruses are transmitted through direct contact, indirect contact, large respiratory droplets and aerosols (droplets nuclei).

Influenza viruses belong to the Orthomyxoviridae family and are divided into types A, B and C. Influenza types A and B are responsible for epidemics of respiratory illness that are often associated with increased rates of hospitalization and death. During the 20th century, the only influenza A subtypes that circulated extensively in humans were (H1N1) Spanish Flu; (H1N2); (H2N2) Asian Flu; and (H3N2) Hong Kong Flu. A new strain of influenza A, H1N1 emerged in 2009 called 'Swine Flu' as it originated in swine and spread to humans. More recently in 2013, a new strain of Avian Influenza A, H7N9 has infected people in China and is believed to be from exposure to infected poultry.

All known subtypes of influenza type A viruses have been isolated from birds and can affect a range of mammalian species. As with humans, the number of influenza A subtypes that have been isolated from other mammalian species is limited. Influenza type B viruses almost exclusively infect humans.

In this case, influenza type A virus has been used for the testing.

## 4. Protocol

---

### 4.1. Test Conditions

Testing of the IQAir HealthPro 250 air purifier, was conducted in a 28.5 m<sup>3</sup> environmental test chamber. The chamber was preconditioned to 20 °C ( $\pm 3$  °C) and 55 % ( $\pm 5$  %) relative humidity before the commencement of the tests. After each run, the chamber was sterilised by operating a UV germicidal lamp, installed in the ceiling of the chamber, for at least 60 minutes. The air was extracted from the test chamber through HEPA filters, and fresh HEPA filtered air was resupplied. The chamber was then cleaned by washing with 5% Virkon multi-purpose disinfectant solution.

### 4.2. Air Purifier Control and Test Runs

Six decay tests were performed in the environmental chamber consisting of:

- Three inactive control runs without the IQAir HealthPro 250 air purifier
- Three active test runs with the IQAir HealthPro 250 air purifier operating at the max airflow


For the active test runs the air purifier was placed on the floor in the centre of the chamber. For the inactive control runs, the same procedure was performed except in the absence of the air purifier. Three replicates per sample timepoint were collected during each run.

In both the active and inactive runs, viable Influenza A virus was aerosolised into the chamber for up to 20 minutes. The amount of Influenza A aerosolised was dependent on the virus stock used, however 100 - 200  $\mu\text{g}$  of virus antigen was introduced into the test chamber for each run. The viral aerosol was mixed in the chamber by a ceiling fan, which was operating at low speed for the duration of the test.

### 4.3. Sampling Time Points

Three SKC BioSamplers collected air samples at 1 m height for 10 minutes at a rate of 11.8 l/min at the following time points:

- -10 to 0 min (AS-1)
- 0 to 10 min (AS-2)
- 10 to 20 min (AS-3)
- 20 to 30 min (AS-4)
- 30 to 40 min (AS-5)

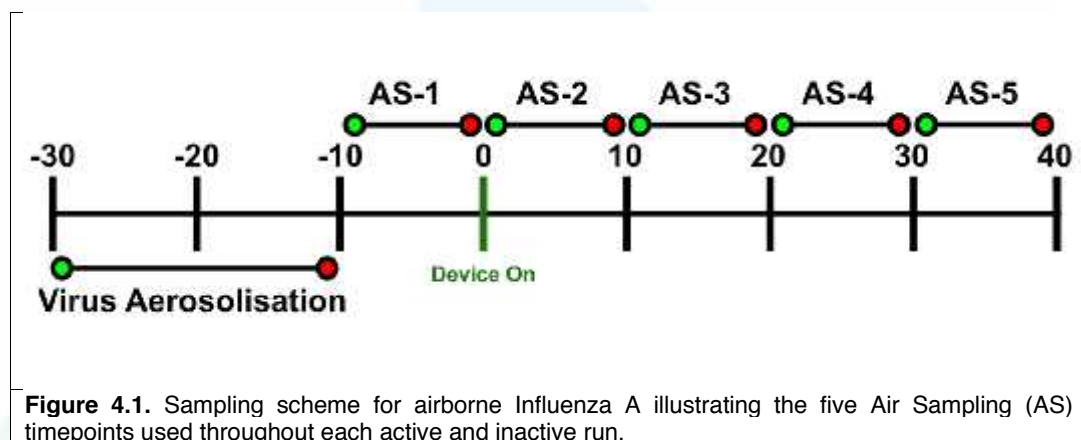

**Figure 4.1.** Sampling scheme for airborne Influenza A illustrating the five Air Sampling (AS) timepoints used throughout each active and inactive run.

For the active test runs, the air purifier was operated remotely at  $t = 0$  minutes and remained operating for the duration of the test (Figure 4.1). At the end of the test, the samples were removed from the BioSamplers and transferred to sterile 40 ml tubes that were immediately placed on ice and then stored in the laboratory at  $-20^{\circ}\text{C}$  until analysis.

### 4.4. Sample Analysis

Influenza A quantification was performed by ELISA. The ELISA (enzyme-linked immunosorbent assay) is a plate-based assay technique that uses antibodies with high specificity to detect and quantify substances, such as peptides and proteins, called antigens. The NCP-ELISA validated at **airmid healthgroup** detects and quantifies Influenza A nucleoprotein (NPA). In this report, the abbreviation “**Inf A**” is used to refer to the virus quantified by the ELISA detection of the **NPA antigen**. The concentration of Inf A in each sample is reported in this report as ng per  $\text{m}^3$  of sampled air.

Virus reduction percentage was calculated according to the formula below:

$$\% \text{ Virus Reduction} = 100 - \frac{\text{InfA ng/m}^3 \text{ with device operating (t = tx min)}}{\text{InfA ng/m}^3 \text{ without device operating (t = 0 min)}} \times 100$$

\* tx = sample timepoint

## 5. Results and Discussion

The recovery concentrations of Inf A in the three inactive control runs and in the three active test runs are reported in Tables 5.1 and 5.2. Each result is the average of three replicates (unless specified otherwise) sampled at the indicated time. The Inf A concentration was determined by ELISA in units of ng/ml and then converted into ng/m<sup>3</sup>, i.e. nanograms of Influenza A per cubic metre of air sampled by the SKC BioSamplers.

**Table 5.1. Average Influenza A concentration measured in the inactive control runs.**

Timepoint	Control 1 ng/m <sup>3</sup>	Control 2 ng/m <sup>3</sup>	Control 3 ng/m <sup>3</sup>
-10 – 0	2320.00*	2857.87*	3196.60*
0 – 10	2289.36*	2643.97	2807.94
10 – 20	1497.87	2230.35	1837.73
20 – 30	1364.26*	1930.21	1788.37
30 – 40	1622.98*	2151.49	1673.76

\* Results generated from averaging 2 sampling replicates

**Table 5.2. Average Influenza A concentration measured in the active test runs.**


Timepoint	Test 1 ng/m <sup>3</sup>	Test 2 ng/m <sup>3</sup>	Test 3 ng/m <sup>3</sup>
-10 – 0	1070.64	1079.15	1130.21
0 – 10	< LOD	< LOD	< LOD
10 – 20	< LOD	< LOD	< LOD
20 – 30	< LOD	< LOD*	< LOD
30 – 40	< LOD	< LOD	< LOD

<LOD: Less than the limit of detection

\* Results generated from averaging 2 sampling replicates


Figures 5.1 and 5.2 show the trend of Inf A levels over time in the three control and test runs, respectively. The rapid reduction in Inf A concentration observed in the test runs (Figure 5.2) could not be attributed to natural decay due to forces exerted on the virus particles, i.e. inertia, diffusion. In the three test runs, between 0 and 10 minutes of the air purifier operating, the Influenza A concentration had dropped below the detection limit of the assay used to quantify the virus. The differences among the same sampling time points in the runs can be ascribed to the virus stock

used to perform the runs and the sampling process itself. As reported by Fabian et al. in 2009, for laboratory studies SKC BioSamplers represent the most efficient airborne virus particle sampling tool in terms of virus infectivity preservation and collection efficiency. Despite this, the BioSampler recovery efficiency is about 79% for particles sized  $> 0.3 \mu\text{m}$ , which may lead to variation in the collected concentrations of Inf A particles sized  $\sim 0.1 \mu\text{m}$ .

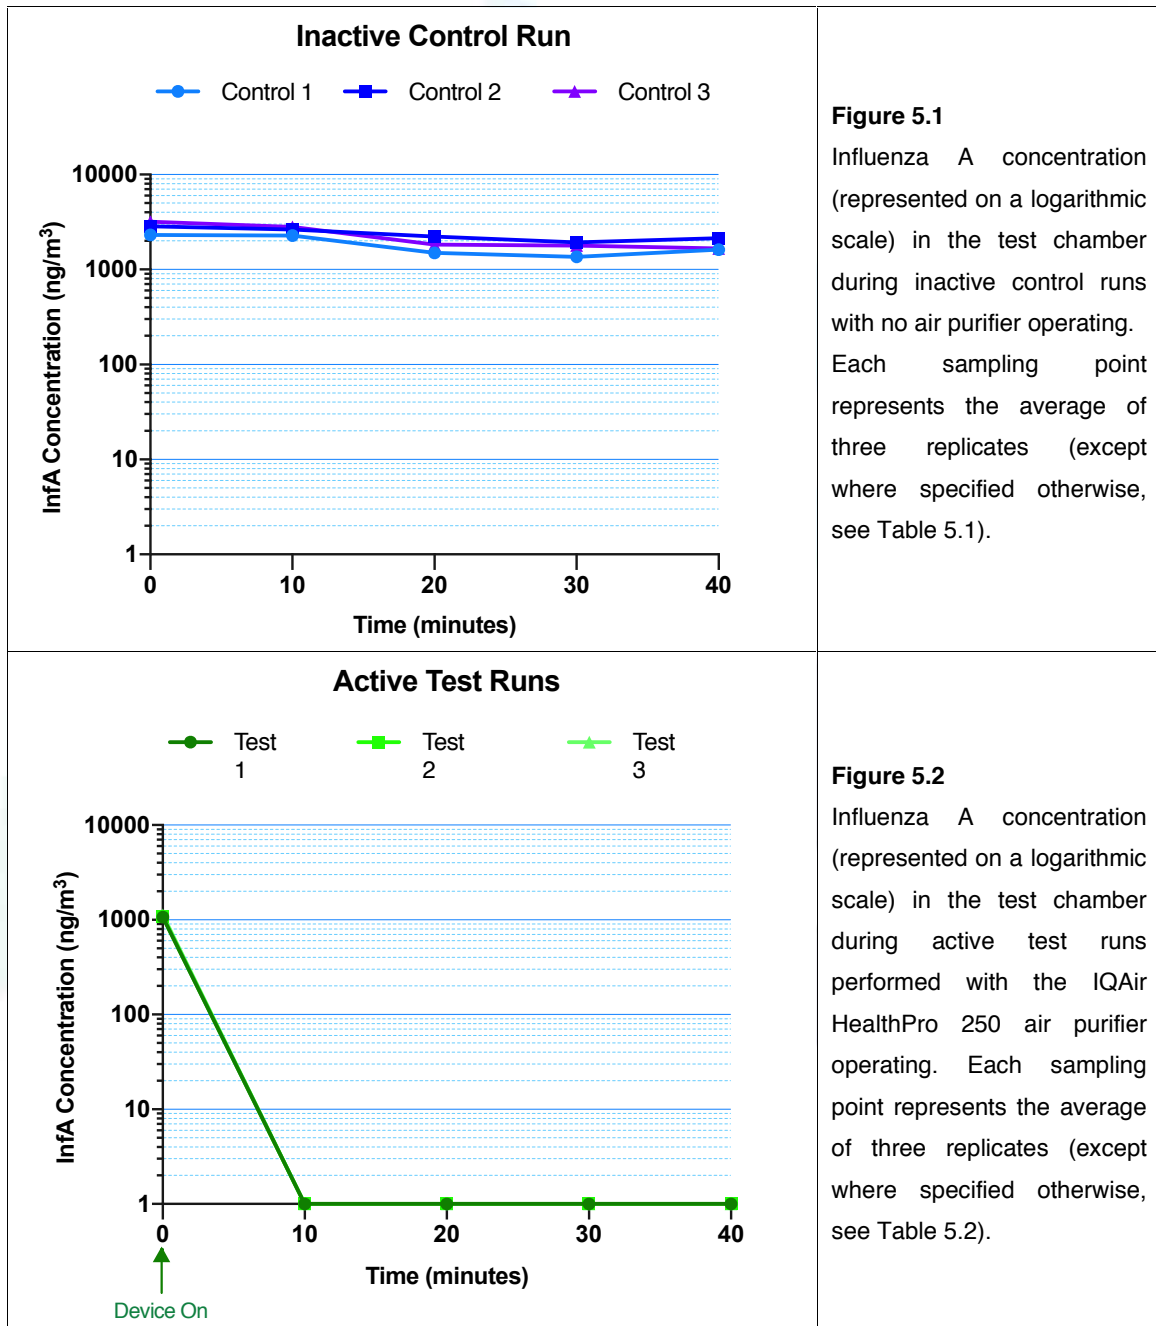

The data presented here show that within the first 10 minutes of the IQAir HealthPro 250 air purifier operating at the highest fan speed, the Influenza A concentration in the test chamber was reduced to less than 0.156 ng/ml (the detection limit of the assay performed to quantify the collected airborne virus).

Figure 5.3 shows the percentage reduction in Inf A levels (calculated per the formula cited above in Section 4.4) during the control and test runs. Fluctuations in virus concentration were observed during control runs. Statistical fluctuations are unavoidable, especially for a test like the one described in this report. Several factors affect the outcome of the result. The sampling process and the assay bring their own variability, and one must not forget that the virus, adapted to the ideal 'survival' environment of the human body, is aerosolized into an indoor space with certain physical characteristics, where physical forces such as inertia and diffusion are applied on the viral particles throughout the test duration (Hind 1999, U.S. EPA 2010, Lee et al. 2011). The aerosolised virus may also adhere to the chamber surfaces after a certain period or move to areas of the chamber with a lower or null concentration of virus, with a consequent variation in the number of particles collected by the SKC BioSamplers over an extended period. In contrast, a 99.9% decrease in Inf A levels is observed in the test runs at the first sampling time after the air purifier is turned on.

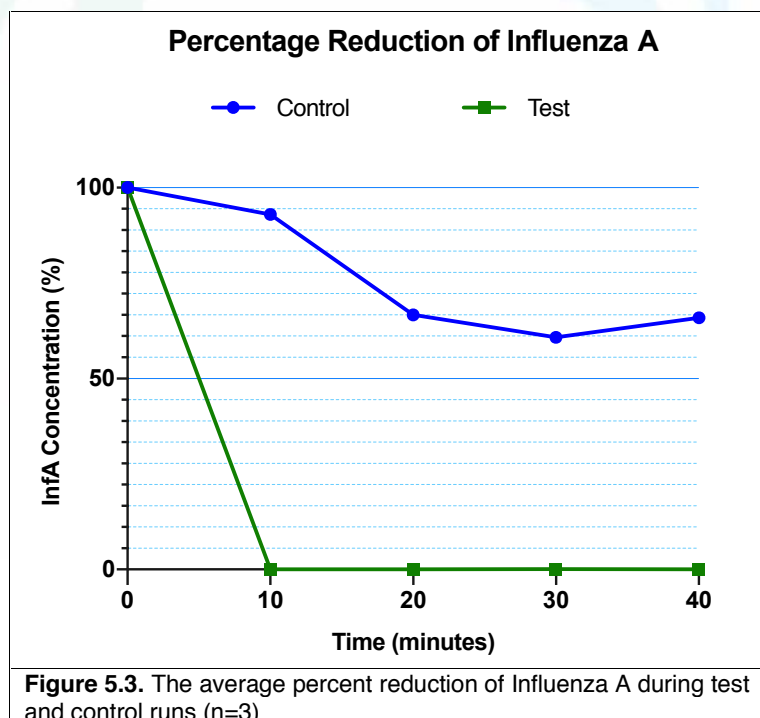



## 6. Conclusion

---

The IQAir HealthPro 250 was demonstrated to be effective in reducing airborne Influenza A aerosols in the test chamber, achieving 99.9 % airborne virus reduction within the first 10 minutes of operation at the highest air flow rate. Influenza A was not detected by ELISA in the air samples at the 0 – 10, 10 – 20, 20 – 30, and 30 – 40 timepoints, collected during active test runs with the air purifier operating. These results indicate that in the presence of an operational unit the Influenza A concentration in the test chamber was reduced to levels below 0.156 ng/ml, the detection limit of the assay performed to quantify the collected airborne virus.

## 7. Additional Products

---

As per the declaration of conformity signed by IQ Air on the 9<sup>th</sup> June 2020, the product listed below conforms in all aspects relating to performance in testing parameters to the IQAir HealthPro 250 air cleaner.

- IQAir HealthPro Plus

## 8. References

---

Hinds (1999). *Aerosol Technology*. John Wiley & Sons, Inc New York / Chichester / Weinheim / Brisbane / Singapore / Toronto.

Fabian P., McDevitt J.J., Houseman E.A., Milton D.K. (2009). An optimized method to detect influenza virus and human rhinovirus from exhaled breath and the airborne environment. *Indoor Air*; 19(5): 433-441.

EPA/600/R-10/127 (2010). *Development of a Methodology to Detect Viable Airborne Virus Using Personal Aerosol Sample*.

Lee I., Kim H., Lee D., Hwang G., Jung G., Lee M., Lim J. Lee B. (2011). Aerosol Particle Size Distribution and Genetic Characteristics of Aerosolized Influenza A H1N1 Virus Vaccine Particles. *Aerosol and Air Quality Research*, 11, 230–237.

## 9. Amendment History

Section	Page(s)	Description of Amendment
7	9	<p>As per the declaration of conformity signed by IQ Air on the 9<sup>th</sup> June 2020, the product listed below conforms in all aspects relating to performance in testing parameters to the IQAir HealthPro 250 air cleaner.</p> <ul style="list-style-type: none"> <li>• IQAir HealthPro Plus</li> </ul>

This report ASCR092408v2 supersedes previous versions.



“This report is provided on a confidential basis for the benefit of airmid healthgroup’s client pursuant to the agreement between airmid healthgroup and its client. A right of action arising under this report cannot be assigned. airmid healthgroup’s responsibility under this report is limited to proven negligence and will in no case be more than the testing fees. The results shown on this test report refer only to the sample(s) tested unless otherwise stated, under the conditions agreed upon. Anyone relying on this report should understand all of the details of the engagement. Only the client is authorised to publish, copy or make this report available to any third party, and then only in its entirety. This report or the airmid healthgroup limited name or logo cannot be included in any materials, including any legal, publicity or advertising activities relating to the tested product or service without the explicit written consent of airmid healthgroup Ltd.”

**Report written by:**

Jake Behan, BSc.  
Head of Operations

**Report reviewed by:**

Vivienne Mahon, PhD.  
Chief Scientist/Quality Director

\*\*\*End of Report\*\*\*